



Quality Club™


Quality Club Specific IgE Monthly Report

Lab Code: 356 005
 Test Period: September 2015
 Sample Lot No.: AWUBH
 System: Phadia 250 (02104)

Results from all labs

N (except outliers) 457
 Median 31,4 kU_A/L
 Mean 31,7 kU_A/L
 SD 3,64 kU_A/L
 CV 11,5 %
 Mean - 2 SD 24,4 kU_A/L
 Mean + 2 SD 38,9 kU_A/L


Your results	29,7 kU_A/L
Deviation from mean	-6,06 %
Deviation score	-0,53

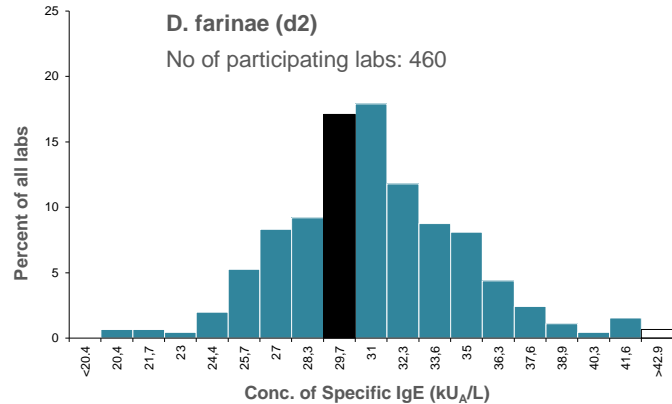

Results from all labs

N (except outliers) 468
 Median 9,54 kU_A/L
 Mean 9,55 kU_A/L
 SD 0,9 kU_A/L
 CV 9,4 %
 Mean - 2 SD 7,75 kU_A/L
 Mean + 2 SD 11,3 kU_A/L

Your results	9,02 kU_A/L
Deviation from mean	-5,58 %
Deviation score	-0,59

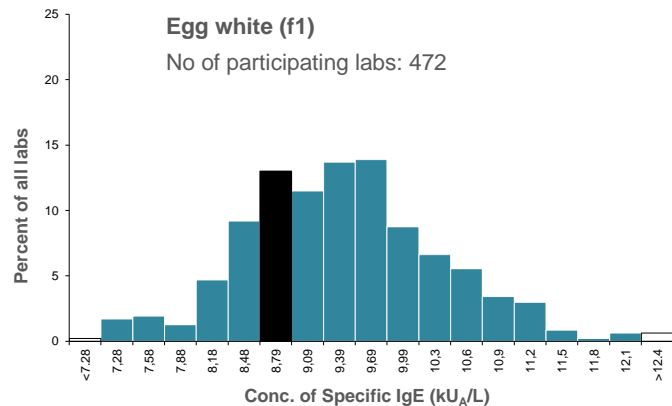

Results from all labs

N (except outliers) 433
 Median 3,55 kU_A/L
 Mean 3,54 kU_A/L
 SD 0,34 kU_A/L
 CV 9,5 %
 Mean - 2 SD 2,87 kU_A/L
 Mean + 2 SD 4,22 kU_A/L

Your results	3,3 kU_A/L
Deviation from mean	-6,82 %
Deviation score	-0,72

